



Challenge

Reproducible and reliable determination of TOC and TN_b contents in samples with high particle loads/wastewater.

Solution

Fully automated and simultaneous TOC/ TN_b measurement using direct injection technology and catalytic high-temperature combustion, which allow optimum particle handling and a minimized risk of carry-over.

TOC/ TN_b Determination in Municipal Sewage Plants

Introduction

In wastewater treatment plants, the organic and nitrogen load have to be measured in the untreated inflow, the pretreated effluent, and the final effluent after the completed treatment process. In many cases, the chemical oxygen demand (COD) and TN contents are measured with separate methods. This is a labor- and time-consuming process often associated with the formation of chromium-VI-contaminated waste. Through correlation studies, an empirical conversion factor for TOC to COD conversion can be established. Hence, a fully automated analytical process for TOC/ TN_b determination according to EN 14848^[1] and EN 12260^[2] can be applied to save resources and time. In order to guarantee accurate and efficient analysis, it is recommendable to use a catalytic high-temperature combustion TOC analyzer for simultaneous determination of NPOC and TN_b from one single injection. According to these standards, TOC is defined as the sum of dissolved and particle-bound organic carbon compounds. Thus, the challenge is to assure a representative sample transfer, including all the particles, into the combustion system and

at the same time to guarantee a complete oxidation of both, difficult-to-oxidize substances and particle-bound organics. This requires an effective sample homogenization on the autosampler rack and a sample introduction technique that ensures no particles get lost on the way to the combustion tube or cause any blockages, which may lead to system downtime or to extended wear and tear on sensitive Teflon parts inside the dosing system. A combustion system capable of providing sufficiently high furnace temperatures to assure a complete sample digestion is required as well. This application note describes a method using the multi N/C 2300 TOC/ TN_b analyzer. The samples were measured at a customer's site (wastewater treatment plant) in Germany using a direct injection system for optimized particle handling.

Materials and Methods

Samples and reagents

- Wastewater samples were taken from the inflow into the sewage plant as well as intermediate treatment stages
- 2 M HCL was used for automatic sample acidification to a pH < 2

Sample preparation

The samples were stored in a refrigerator at 4 °C until analysis and then transferred into suitable autosampler vials. The wastewater samples were analyzed in direct mode applying an NPOC/TN_b method. The samples were adjusted to pH < 2 using 2 M HCl, and subsequently purged for a period of 5 minutes. An injection volume of 250 µL was used for these measurement sequences. The samples were catalytically oxidized at a temperature of 800 °C in an oxygen

flow. The 16 mm combustion tube, filled with platinum catalyst was used. The formed nitrogen oxides are detected by means of a chemiluminescence detector (alternatively a ChD detector can be utilized), CO₂ detection was done by FR-NDIR.

Calibration

The multi N/C analyzer was calibrated between 1 and 1,000 mg/L for total organic carbon (TOC) with a potassium hydrogen phthalate standard solution. A multipoint calibration was used to evaluate the results of the NPOC measurement. For total bound nitrogen a calibration was carried out from 1 to 100 mg/L with an ammonium sulfate and potassium nitrate solution (50:50 mix) according to EN 12260.

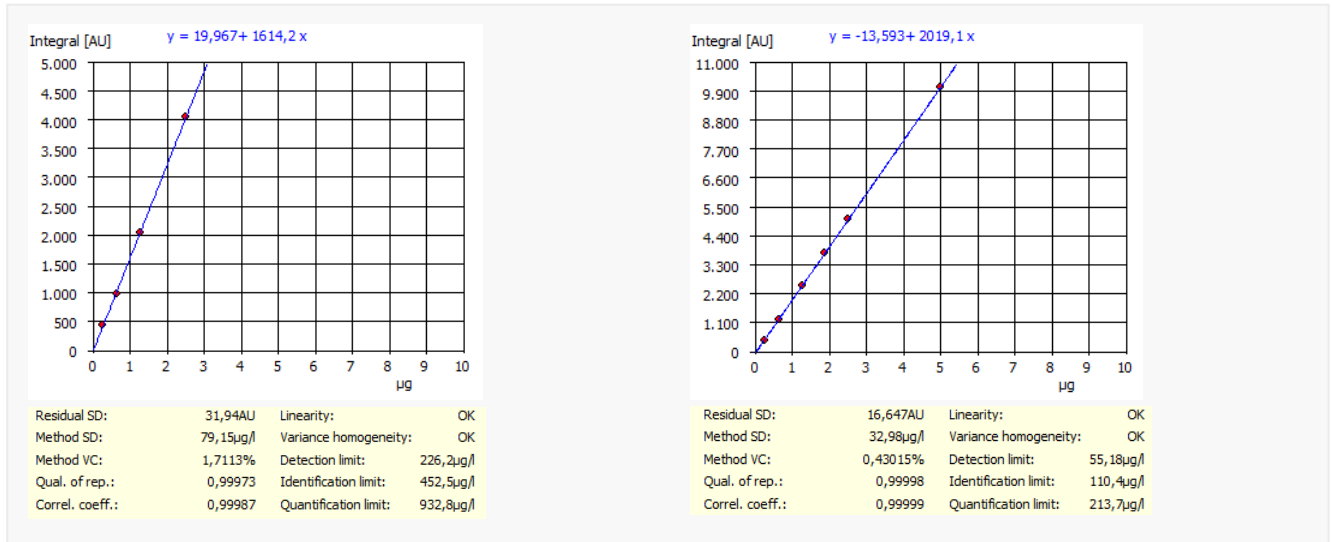


Figure 1 and 2: Example of TC and TN calibration and method characteristics

Within the method up to three calibration ranges can be linked to each parameter in order to cover an over-all working range of up to three magnitudes.

With the NPOC/TN_b method three NPOC and two TN_b multi-point calibration ranges were linked as follows:

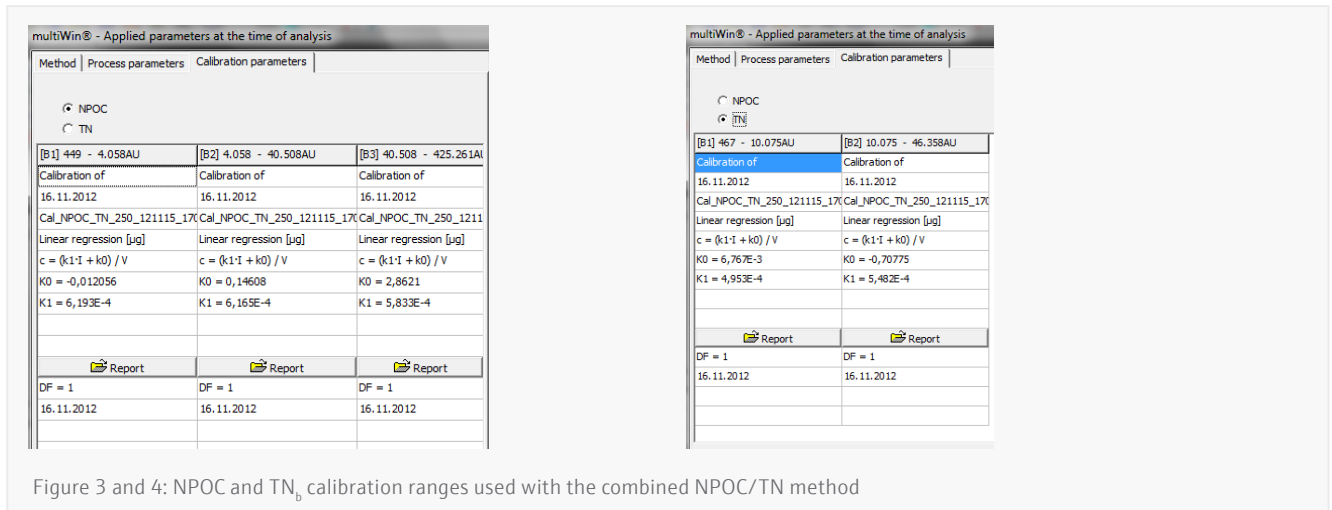


Figure 3 and 4: NPOC and TN_b calibration ranges used with the combined NPOC/TN method

Instrumentation

The following method settings were used to determine the NPOC and TN_b contents:

Table 1: Method settings

Parameter	multi N/C 2300
Measurement parameter	NPOC / TN _b
Digestion	High temperature digestion at 800°C with platinum catalyst
Number of repetitions	min. 3, max. 4
Rinse with sample before injection	3 times
Sample purge time	300 sec.
Injection volume	250 µL

Results and Discussion

The figure below shows the mean values of three replicate injections with relative standard deviations for different real samples (anonymized) and various recovery checks for different TN, TOC and particle suspension reference solutions (cellulose according to EN 1484, annex C), respectively.

Sample ID	Method	TC/NPOC	TN
TC 10mg/l	NPOC TN 250	10.07mg/l ± 0.50%	283.0µg/l ± 1.79%
Cellulose	NPOC TN 250	99.29mg/l ± 0.13%	113.6µg/l ± 2.26%
TC 150mg/l	NPOC TN 250	150.0mg/l ± 0.09%	174.2µg/l ± 3.11%
NO3 NH4 6mg/l	NPOC TN 250	815.0µg/l ± 9.50%	5.96mg/l ± 0.35%
TN 6mg/l	NPOC TN 250	11.68mg/l ± 0.83%	5.96mg/l ± 0.11%
TN 30mg/l	NPOC TN 250	51.17mg/l ± 0.30%	29.29mg/l ± 1.31%
████████	NPOC TN 250	93.79mg/l ± 2.08%	25.37mg/l ± 1.21%
████████	NPOC TN 250	250.7mg/l ± 0.68%	116.3mg/l ± 0.54%
████████	NPOC TN 250	160.2mg/l ± 1.41%	12.12mg/l ± 0.92%
████████	NPOC TN 250	125.2mg/l ± 1.44%	28.53mg/l ± 0.51%
TC 10mg/l	NPOC TN 250	10.40mg/l ± 0.49%	196.2µg/l ± 3.17%
Cellulose	NPOC TN 250	106.6mg/l ± 0.48%	97.80µg/l ± 7.26%
TC 150mg/l	NPOC TN 250	151.4mg/l ± 0.17%	136.2µg/l ± 3.93%
NO3 NH4 6mg/l	NPOC TN 250	432.0µg/l ± 17.45%	6.07mg/l ± 0.34%
TN 6mg/l	NPOC TN 250	11.78mg/l ± 0.96%	6.01mg/l ± 0.93%
TN 30mg/l	NPOC TN 250	51.82mg/l ± 0.07%	29.71mg/l ± 0.94%
████████	NPOC TN 250	49.34mg/l ± 0.74%	22.52mg/l ± 1.33%
████████	NPOC TN 250	230.1mg/l ± 0.47%	93.07mg/l ± 0.71%
████████	NPOC TN 250	887.8mg/l ± 0.35%	59.52mg/l ± 0.75%
████████	NPOC TN 250	221.2mg/l ± 0.64%	116.2mg/l ± 0.51%
TC 10mg/l	NPOC TN 250	9.89mg/l ± 0.11%	145.4µg/l ± 5.26%
Cellulose	NPOC TN 250	100.1mg/l ± 0.65%	141.3µg/l ± 1.91%
TC 150mg/l	NPOC TN 250	150.3mg/l ± 0.10%	93.88µg/l ± 2.42%
NO3 NH4 6mg/l	NPOC TN 250	375.6µg/l ± 5.64%	6.01mg/l ± 0.34%
NO3 NH4 30mg/l	NPOC TN 250	340.3µg/l ± 5.13%	29.40mg/l ± 0.06%
TN 6mg/l	NPOC TN 250	11.64mg/l ± 0.62%	6.02mg/l ± 0.90%
TN 30mg/l	NPOC TN 250	52.02mg/l ± 0.47%	29.76mg/l ± 0.67%
████████	NPOC TN 250	1.04g/l ± 0.30%	23.53mg/l ± 0.59%
████████	NPOC TN 250	104.5mg/l ± 2.25%	90.65mg/l ± 0.67%
████████	NPOC TN 250	996.7mg/l ± 0.77%	13.59mg/l ± 1.26%
████████	NPOC TN 250	284.7mg/l ± 0.86%	158.4mg/l ± 0.81%

Figure 5: Results

Summary

The measurements covered the analysis of undiluted wastewater samples with TOC concentrations up to almost 1 g/L and TN_b concentrations up to 160 mg/L. The analyses were performed with outstanding accuracy and precision. The cellulose test to check for particle handling according to EN 1484, as well as measurements of analytical quality assurance (AOA) standards for TOC and TN_b were performed frequently and showed convincing recovery rates. Especially the recoveries for 6 mg/L and 30 mg/L nicotinic acid TN_b standards prove a high performance for organically bound nitrogen.

The outstanding performance of multi N/C analyzers for matrices such as wastewater is based on the optimized combustion process with freely selectable combustion temperatures up to 950 °C. The direct injection with a septum-free pneumatic injection head in combination with a wide-bore needle of 0.7 mm inner diameter, as well as proper sample homogenization on the autosampler rack and the valve- and tubing-free sample transfer into the combustion system further contribute to this performance. An operation mode keeping the stainless-steel injection needle in the oven head at elevated temperatures during peak integration time to assure complete evaporation of TOC components and a clean needle for further sample processing in combination with an effective rinsing of the microliter injection syringe minimize carry-over effects.

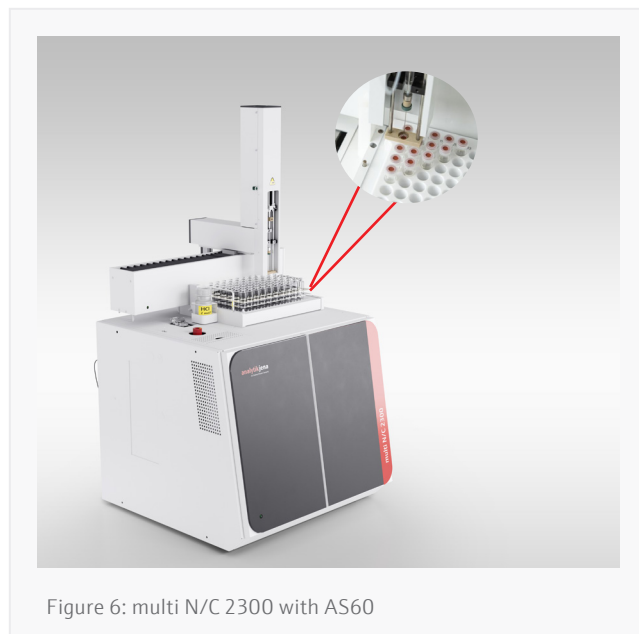


Figure 6: multi N/C 2300 with AS60

A high degree of automation combined with the well-proven Self Check System for trouble free unattended system operation make light work of TOC/TN_b analyses even in challenging samples. In addition, the patented VITA flow management system compensates flow fluctuations inside the system caused by sample evaporation, providing TOC calibration stability for up to one year and saving valuable measurement time.

References

- [1] EN 1484 Water analysis – Guidelines for the determination of total organic carbon (TOC) and dissolved organic carbon (DOC)
- [2] EN 12260 Water quality – Determination of nitrogen Determination of bound nitrogen (TN_b) following oxidation to nitrogen oxides

This document is true and correct at the time of publication; the information within is subject to change. Other documents may supersede this document, including technical modifications and corrections.

Trademark notice: The brand names of the third-party products specified in the application note are usually registered trademarks of the respective companies or organizations.

Headquarters

Analytik Jena GmbH+Co. KG Phone +49 3641 77 70 info@analytik-jena.com
Konrad-Zuse-Strasse 1 Fax +49 3641 77 9279 www.analytik-jena.com
07745 Jena · Germany

Version 2.0 · Author: BeBl
en · 09/2024

© Analytik Jena GmbH+Co. KG | Picture p. 1 ©: iStock/DmitriMaruta